

MD

METABOLIC DISORDERS

LIAISON[®] 25 OH VITAMIN D TOTAL Assay

FOR OUTSIDE
THE US AND
CANADA ONLY

DiaSorin

The Diagnostic Specialist

What is Vitamin D?

LIAISON® 25 OH Vitamin D Total Assay


Vitamin D is a steroid hormone that is produced in the skin upon UV-B exposure or is ingested via the diet.

The 25-hydroxyvitamin D (25 OH Vitamin D) is the most common form of the hormone in the circulation and is the inactive precursor of the active form, 1,25-dihydroxyvitamin D (1,25 (OH)₂ Vitamin D). Because of its long half-life and high concentration, 25 OH Vitamin D is commonly measured for monitoring the Vitamin D status in the patient.


Vitamin D is maintained in the body thanks to two mechanisms, one endogenous, with the production of the hormone thanks to sun exposure and one exogenous, with the introduction of vitamin D with the food. The chemical structures of these types of Vitamin D are different and are called Vitamin D₂ (ergocalciferol) and Vitamin D₃ (cholecalciferol). D₂ is present in some foods and food supplements. Vitamin D₃, on the other hand, is produced by the body at the skin level under the influence of solar radiation. In Vitamin-based pharmaceutical preparations the two forms of Vitamin are indifferently present. The two forms of Vitamin D₂ and D₃ have the same effect and therefore it is important to know the sum of their quantities or the total concentration of 25 OH Vitamin D.

The concentration of 25 OH Vitamin D is used to estimate the reserve of Vitamin D.

Sources and forms of Vitamin:

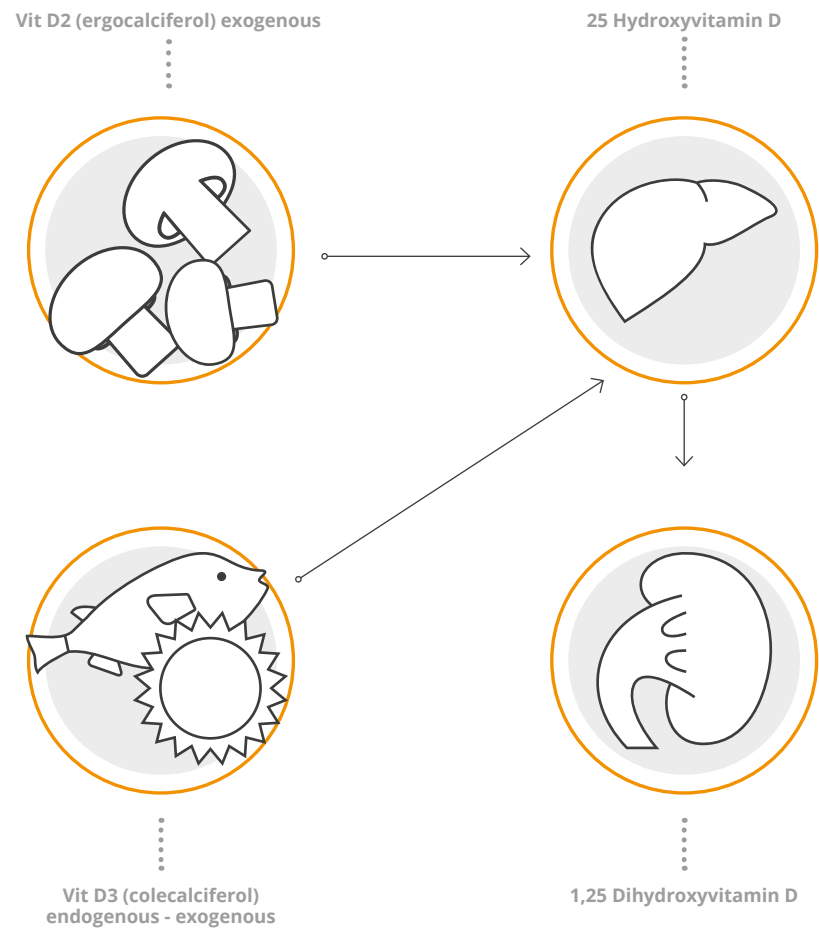


Average Vitamin D in adults (>18 years) around the world

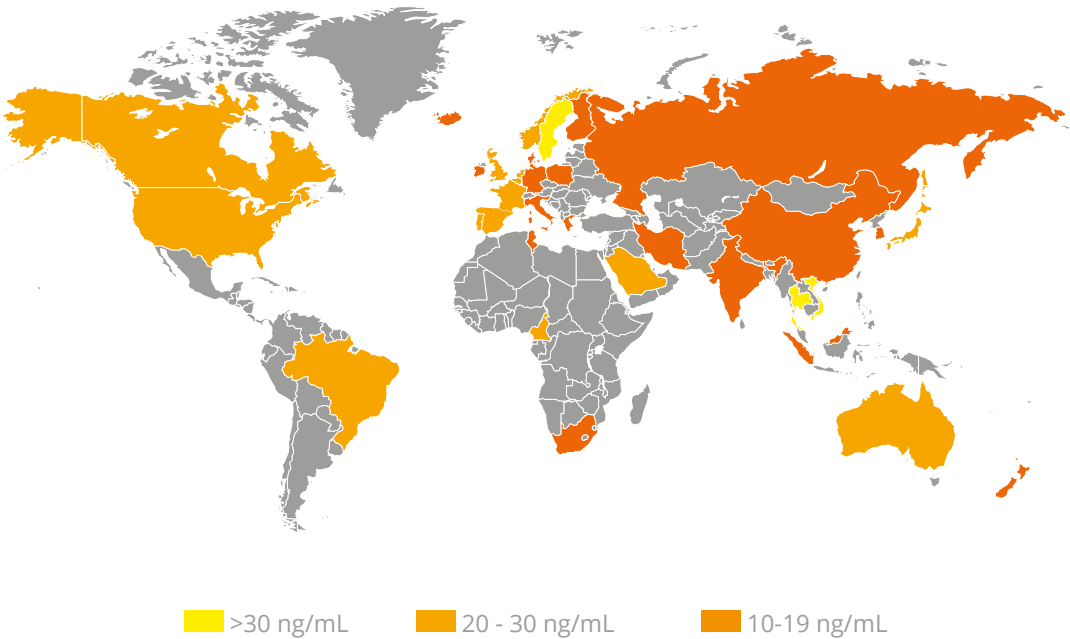

Adapted from Wahl et al. Arch Osteoporos (2012) 7:155-172

Health Based Reference Values as per LIAISON® Vitamin D Total IFU

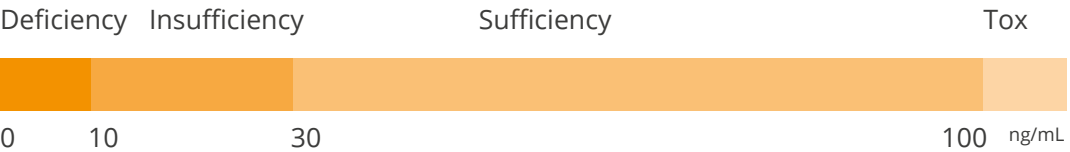

Why 25OH Vitamin D level is relevant for health status

25OH Vitamin D status is an important indicator of health which is investigated in several diseases and conditions. Vitamin D is involved in the homeostasis of calcium and phosphorus and in bone metabolism. An inadequate level of 25OH Vitamin D can lead to a reduction of calcium and phosphorus in the blood circulation, which indirectly stimulate the release of calcium from the bone matrix and the increase of phosphate-wasting in the urine. This results in abnormalities of bone structure in children, muscle and bone weakness and increase falls in the elderly. The monitoring of vitamin D is helpful in those diseases where calcium and phosphorus homeostasis or bone metabolism are altered, like rickets, osteomalacia, osteoporosis and patients with risk of falls and history of fractures, chronic kidney diseases patients, patients with malabsorption disorders, hepatic failure, patients under treatments with some medications and in granulomatosis diseases. Other individuals can suffer of Vitamin D deficiency and monitoring of the values are helpful, like pregnant and lactating women, obese people and afro-american and hispanic people*.

*Holick et al., Evaluation, Treatment and Prevention of Vitamin D Deficiency: an Endocrine Society Clinical Practice Guideline. J Clin Endocrinol Metab, July 2011, 96(7):1911-1930


A Story of Quality

- A fully automated immunoassay for the direct measurement of 25 OH Vitamin D total levels in human serum, EDTA plasma and lithium heparin plasma.
- Allows quick and reliable determination of Vitamin D status and effective therapy monitoring.
- Uses advanced chemiluminescence technology with magnetic microparticle separation to achieve the best assay sensitivity and precision.



CDC Vitamin D Standardization and Certification Program

LIAISON® 25OH Vitamin D Total Assay is certified since 2014.

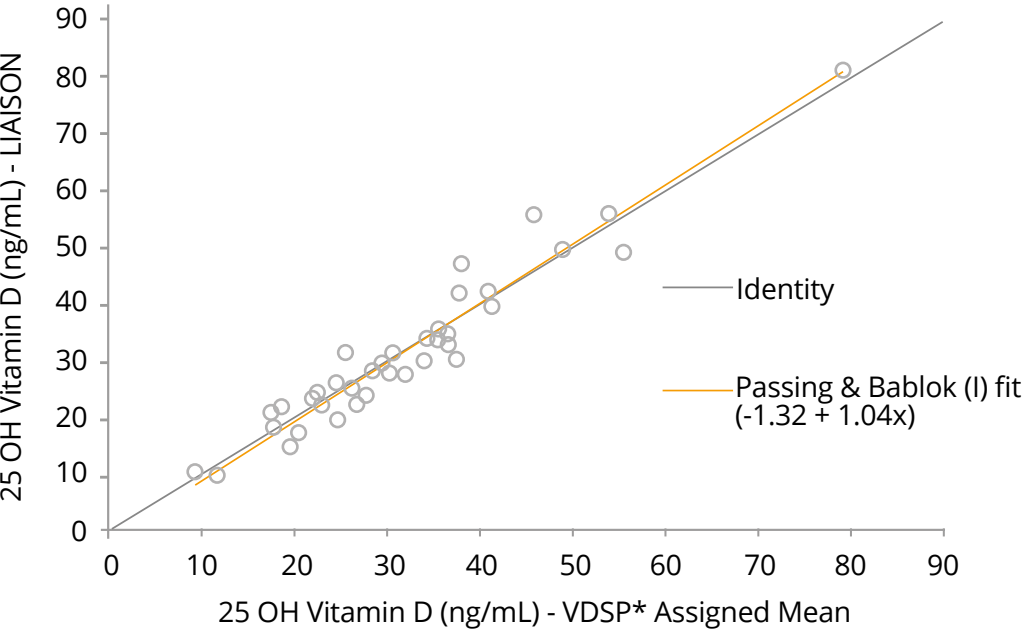


Scatter Plot with Passing & Bablok Fit (N = 40)

VDSCP: Vitamin D Standardization and Certification Program

The scatter plot generated with a Passing & Bablock regression obtained a fit of $y=1.04x -1.32$ vs the VDSP assigned mean, showing an excellent correlation to the DiaSorin 25 OH Vitamin D CLIA assay

The history of DiaSorin Vitamin D test

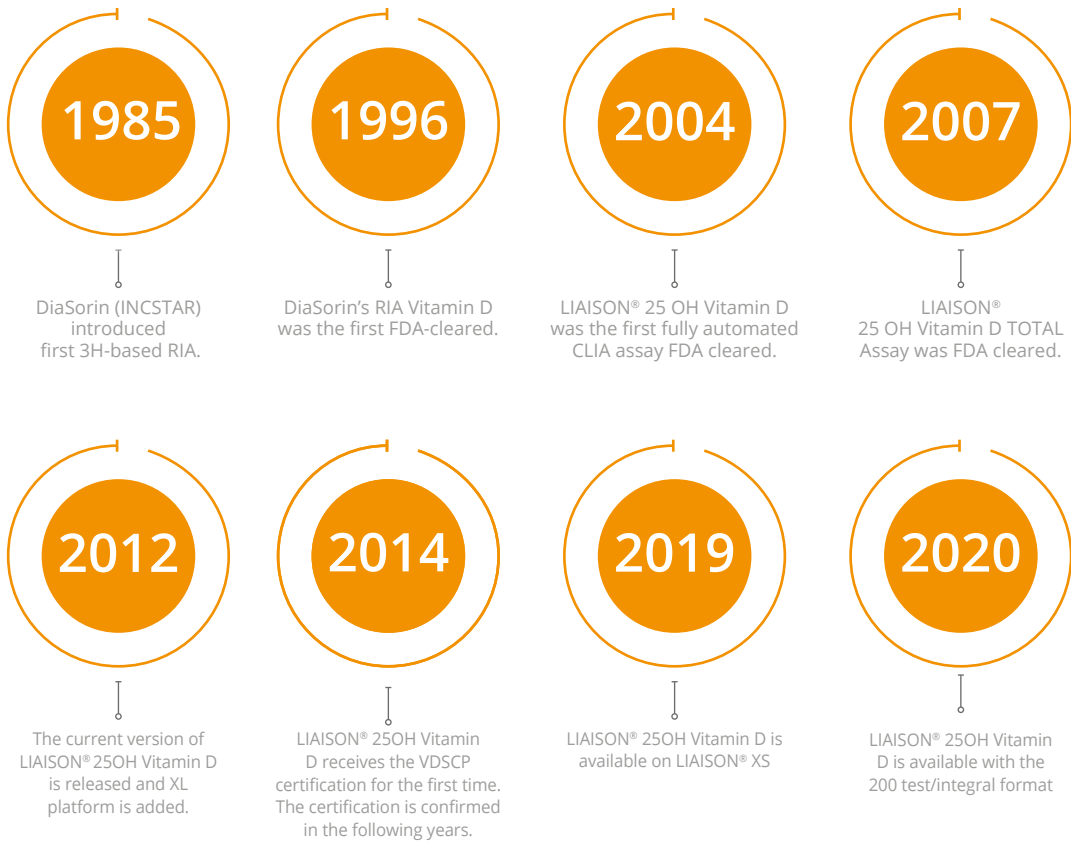

Functional Sensitivity

Guidelines	evaluated according to CLSI EP17-A
Definition	dose concentration at which the % CV exceeds 20%
Sample concentration	2-14 ng/mL
Assays	multiple runs performed
Result	Functional Sensitivity: ≤ 4.0 ng/mL


Cross-reactivity

Guidelines	Evaluated according to CLSI EP7-A2
Sample concentration	spiking up to 100 ng/mL of the potential cross-reactant
Assays	cross-reactivity normalized to 25 OH Vitamin D3
Molecule	Cross-reactivity %
25 OH Vitamin D2	100.0
25 OH Vitamin D3	100.0
Vitamin D2	1.9
Vitamin D3	1.9
1,25 (OH) ₂ Vitamin D2	6.7
1,25 (OH) ₂ Vitamin D3	9.3
3-epi-25 OH Vitamin D3	1.3

Assay precision

Guidelines	evaluated according to CLSI EP5-A2			
# samples	6 samples + 2 controls			
LIAISON®	Intra Run Across Lots and Sites		Total Across Lots and Sites	
	SD	% CV	SD	% CV
	2.0	5.4	4.1	10.6
	Intra Run Within One Lot and Site		Total Within One Lot and Site	
	SD	% CV	SD	% CV
	1.7	4.9	3.8	7.8
LIAISON® XL	Intra Run		Total	
	SD	% CV	SD	% CV
	0.8	2.3	3.8	7.80

LIAISON® 25 OH Vitamin D TOTAL Linearity Serum and SST

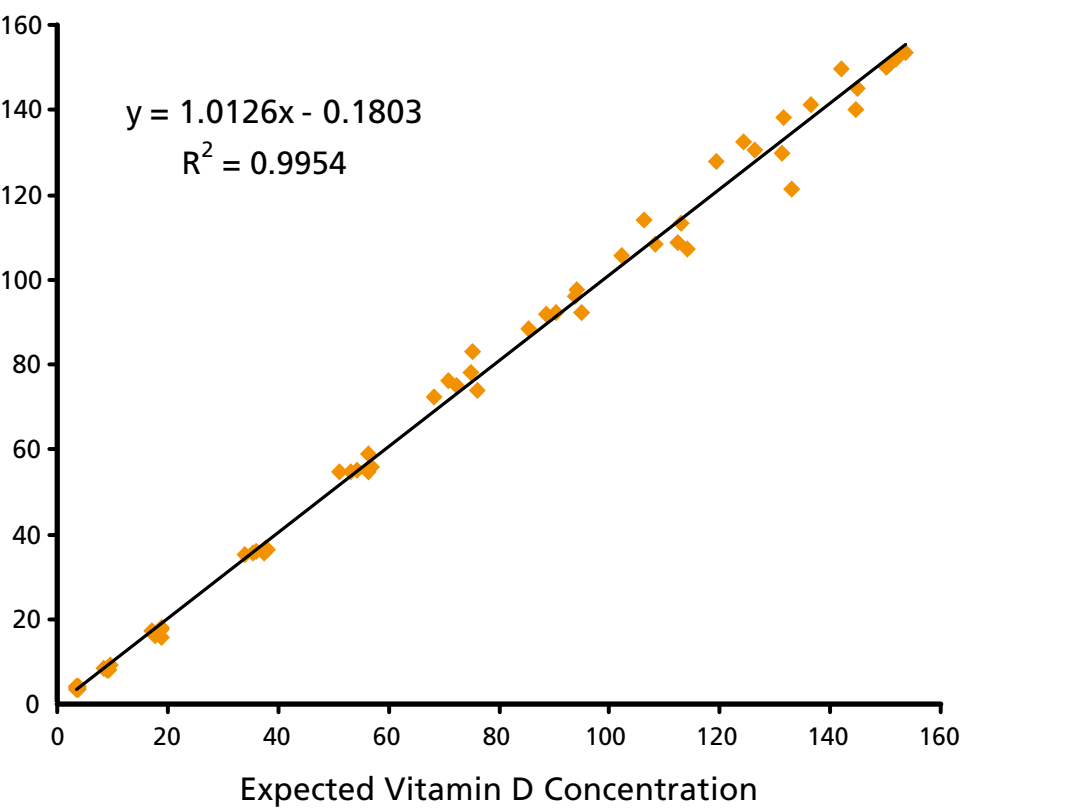

DiaSorin: The Diagnostic Specialist in Vitamin D

25 OH Vitamin D TOTAL		
Part Number	310600	318360
Determinations per Reagent Integral	100	200
Instrument Assay ID	25OHD	25OHD2
Instrument Compatibility	LIAISON®, LIAISON® XL, LIAISON® XS	LIAISON® XL
Reagent Integral Open Stability	4 weeks	
Calibration Stability	7 days	
Assay Range	4.0 - 150 ng/mL	

Ordering information

LIAISON® 25 OH Vitamin D TOTAL Assay 100 test	code 310600
LIAISON® 25 OH Vitamin D TOTAL Assay 200 test	code 318360*
LIAISON® 25 OH Vitamin D TOTAL Control Set	code 310601
LIAISON® 25 OH Vitamin D TOTAL Specimen Diluent Set	code 310602

Please visit: **www.diasorin.com**
for more information and updates

LIAISON® is a registered trademark of DiaSorin

Available on LIAISON® Analyser family

***Available on LIAISON® XL only**

Product availability subject to required regulatory approval

Diasorin Australia Pty Ltd

Building B, Suite 1, Level 4, 11 Talavera Road, Macquarie Park NSW 2113
www.diasorin.com